




Option number can be found inside the battery compartment.

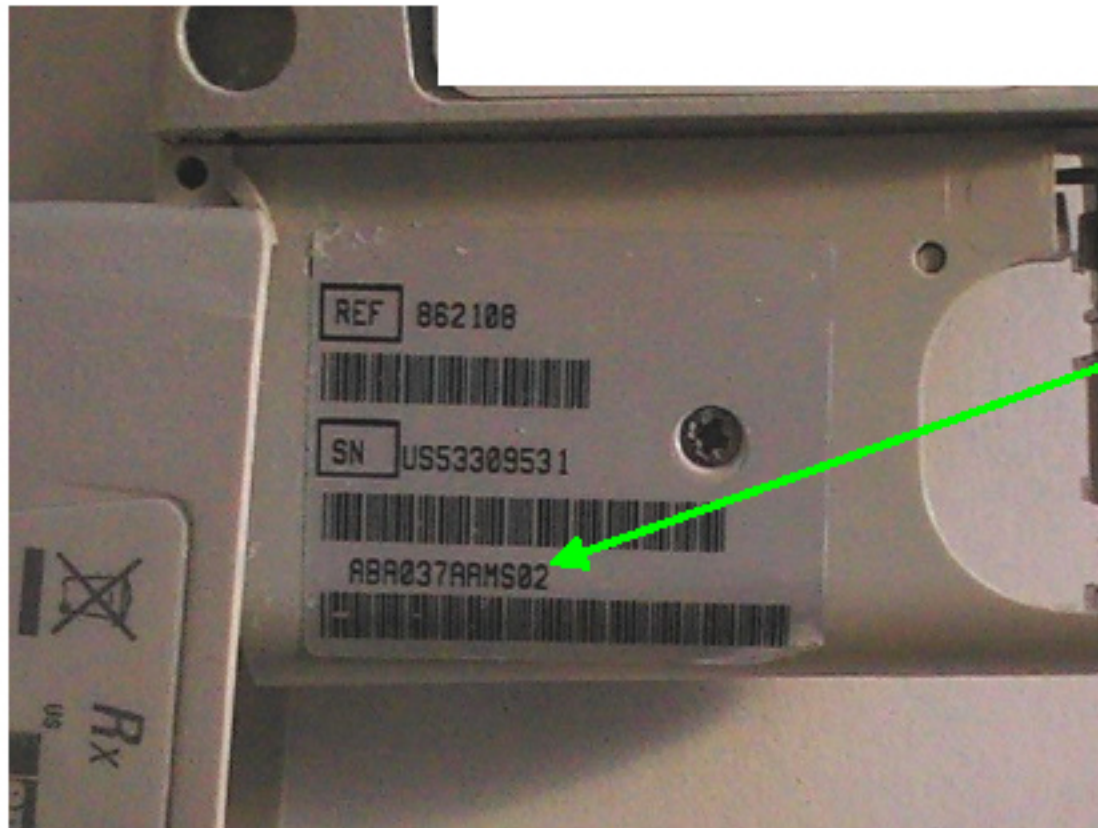

S01= ECG Only
S02=ECG and SpO₂
S03=ECG Only with
upgradeability to SpO₂

BMES *It Has To Be Right!*
Bio-Medical Equipment Service Co.
1-888-828-2637